




Date: Aug.07,2020 Date of Receipt: Jul.15,2020 TEST REPORT TUCHENG ORIGINAL  
 Report No.: TFF9G400 Quantity: 1PC (P1/3) Ref. No.: NIL  
KAO CHEN ENTERPRISE CO., LTD.(U3124) Mask  
 Report Title: \_\_\_\_\_ Item: \_\_\_\_\_  
2F., No. 73, Ln. 308, Sangang Rd., Longjing Dist., Taichung City 43444, Taiwan (R.O.C.)  
 Address: \_\_\_\_\_

Test Items	Test Results	Test Methods
Air Exchange Pressure (mmH2O/cm <sup>2</sup> )	1	4.4
	2	3.5
	3	3.1
	4	2.6
	5	4.3
		CNS 14774 T5017-2018 9.4 CNS 14777 T4039-2003

Note: Air Exchange Pressure takes 5 masks for testing.

Note: Sample description is given by the client: "SOFTGUARDS" disposable medical mask

Note: The test report is the test results issued by the testing institution as requested by the consignor, it shall not determine the legitimacy of the product.

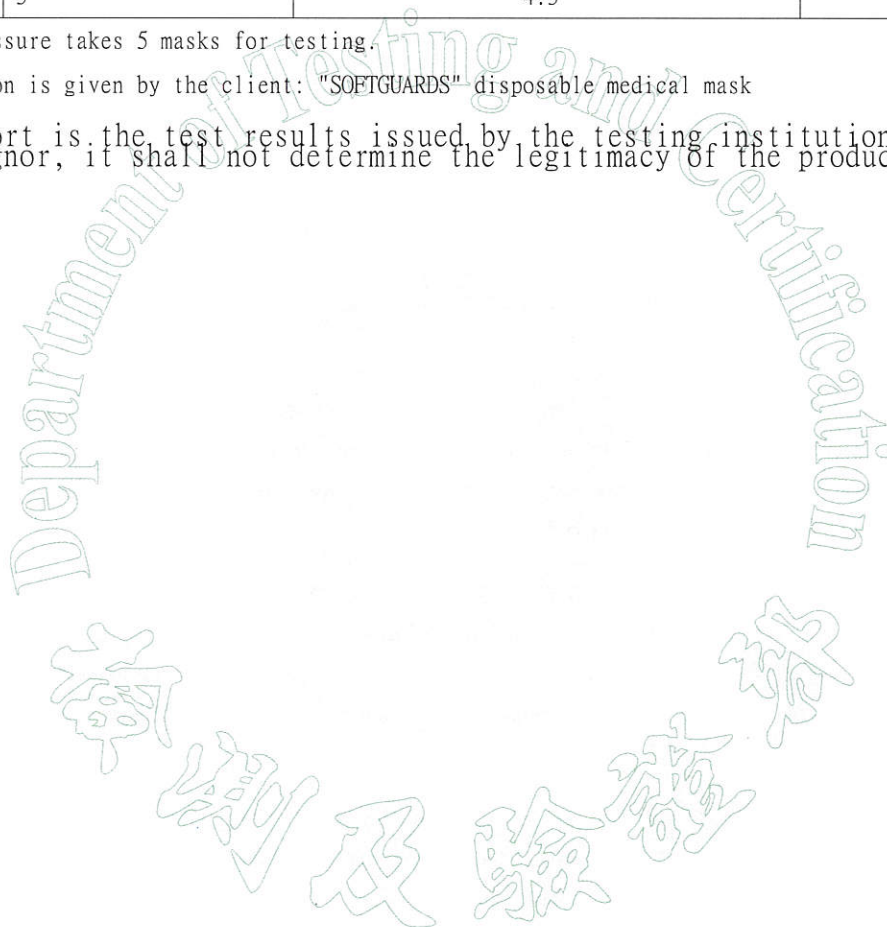

- Note: 1.This report is only responsible for the submitted sample(s), which will be kept for one month period.
- 2.This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.
- 3.The test report should not be used for public advertisement and commercial promotion.

Authorized by president of  
Taiwan Textile Research Institute

*Jui-hung kao*

Director,  
Department of Testing and Certification

Department of Testing and Certification, Taiwan Textile Research Institute  
 No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R.O.C.)  
 Tel : +886-2-22670321 ext. 7107, 7110  
 Fax : +886-2-22675108 , +886-2-22689839



Date: Aug. 07, 2020 Date of Receipt: Jul. 15, 2020

TEST REPORT

TUCHENG

ORIGINAL

Report No.: TFF9G400 Quantity: 1PC (P2/3) Ref. No.: NIL  
KAO CHEN ENTERPRISE CO., LTD.(U3124) Mask

Report Title: 2F., No. 73, Ln. 308, Sangang Rd., Longjing Dist., Taichung City 43444, Taiwan (R.O.C.) Item:

Address:

Test Items		Test Results	Test Methods
Bacterial Filtration	1	99.7	CNS 14774-T5017-2018 9.2
Efficiency (BFE)(%)	2	99.3	CNS 14775 T4037-2003
Staphylococcus aureus	3	99.4	
ATCC 6538	4	99.2	
	5	99.2	

Note: Control average: 1826 CFU.

Note: Mean particle size: 3.1  $\mu$ m.


Note: Testing side: outside of specimen.

Note: Testing area: 39.5 cm<sup>2</sup>.

Note: Flow rate : 28.3 L/min.

Note: Sample description is given by the client: "SOFTGUARDS" disposable medical mask

Note: The test report is the test results issued by the testing institution as requested by the consignor, it shall not determine the legitimacy of the product.

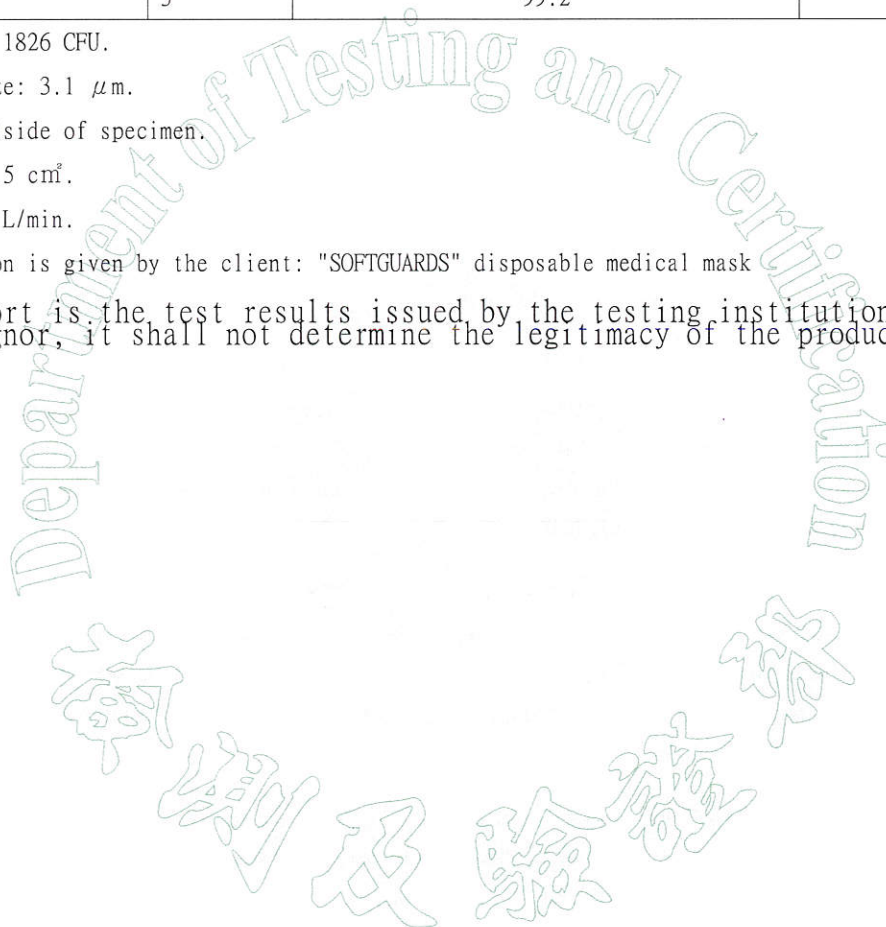

Note: 1.This report is only responsible for the submitted sample(s), which will be kept for one month period.

2.This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.

3.The test report should not be used for public advertisement and commercial promotion.

Authorized by president of  
Taiwan Textile Research Institute

*Jui-hung Kao*

Director,

Department of Testing and Certification

Department of Testing and Certification, Taiwan Textile Research Institute  
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R.O.C.)

Tel : +886-2-22670321 ext. 7107, 7110

Fax : +886-2-22675108 , +886-2-22689839






Date: Aug. 07, 2020 Date of Receipt: Jul. 15, 2020 TEST REPORT TUCHENG ORIGINAL

Report No.: TFF9G400 Quantity: 1PC (P3/3) Ref. No.: NIL

KAO CHEN ENTERPRISE CO., LTD.(U3124) Item: Mask

Report Title: 2F., No. 73, Ln. 308, Sangang Rd., Longjing Dist., Taichung City 43444, Taiwan (R.O.C.)

Address: \_\_\_\_\_

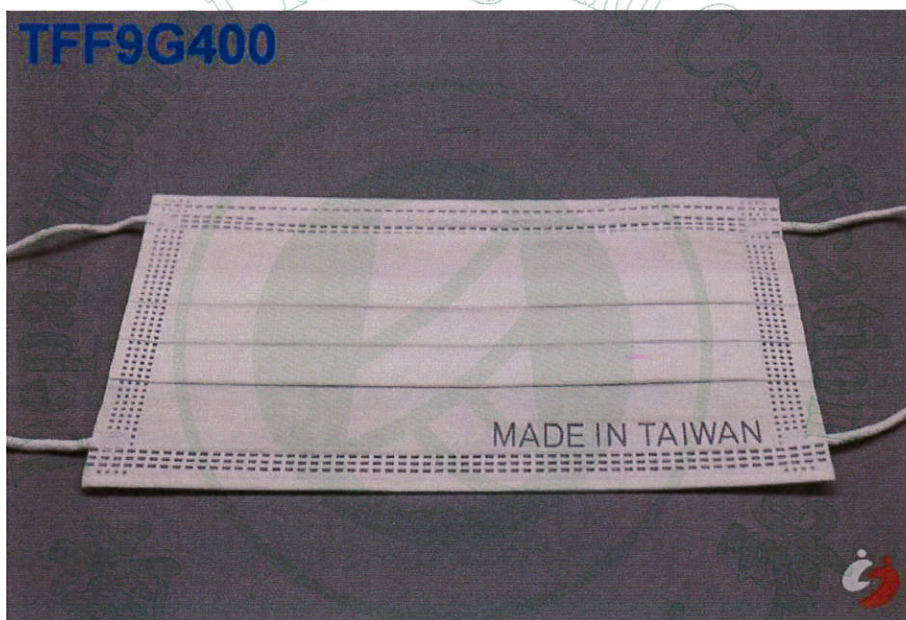

- Note: 1.This report is only responsible for the submitted sample(s), which will be kept for one month period.
- 2.This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.
- 3.The test report should not be used for public advertisement and commercial promotion.

Authorized by president of  
Taiwan Textile Research Institute

*Jui-hung Kao*

Director,  
Department of Testing and Certification  
Department of Testing and Certification  
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R.O.C.)  
Tel : +886-2-22670321 ext. 7107, 7110  
Fax : +886-2-22675108 , +886-2-22689839